Print on Plain White Paper (Part No. 122919)

MIDMARK®

Installation/Operation Instructions

9A10500X Pelvic Lift Assembly

KIT COMPONENTS

Part Number	Description	Qty.
9A10500X	Pelvic Lift Assembly	1
003-0530-00	Installation / Operation Instructions	1

REQUIRED TOOLS

Phillips screwdriver

IMPORTANT INFORMATION

To assist in positioning patients for pelvic examinations.

INSTALLATION (1)

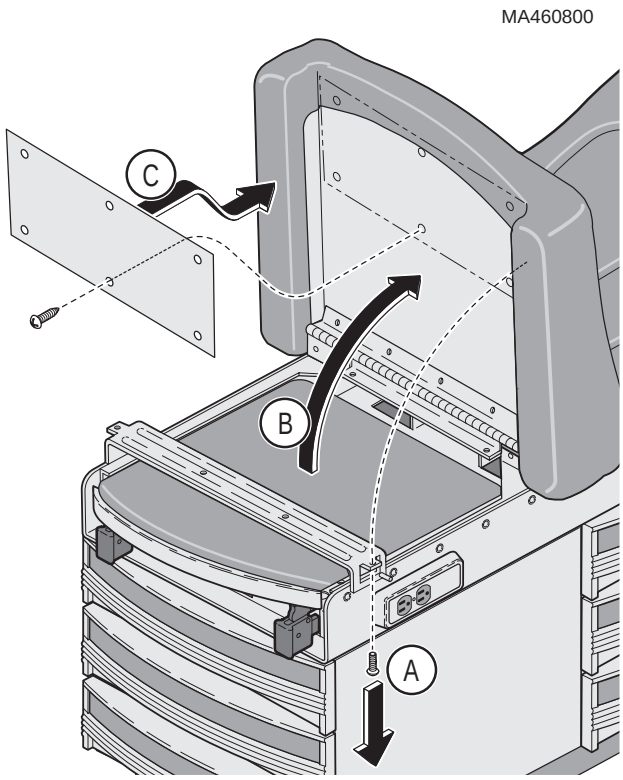

A. Remove two screws that secure seat to upper wrap.
B. Lift seat and secure it to prevent it from falling.
C. Position scuff plate flush against end board of seat section and secure with six #6 x 1/2" self-tapping screws.

INSTALLATION (2)

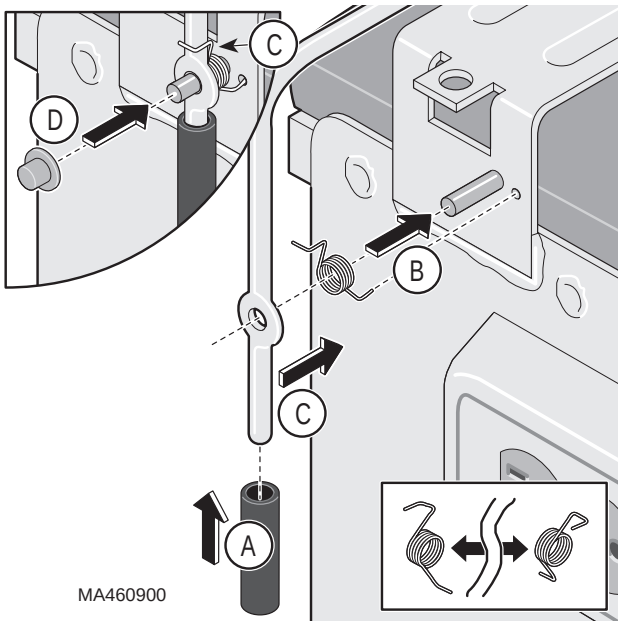

NOTE

There is a right and left-hand spring for pelvic lift bar. "L" shaped end of spring fits into hole on upper wrap. "U" shaped end fits around pelvic lift bar.

A. Install end caps on pelvic lift bar.
B. Install two springs on pivot studs of cross support.
C. Install pelvic lift bar on pivot studs and connect springs.
D. Install push nuts on pivot studs.

OPERATION

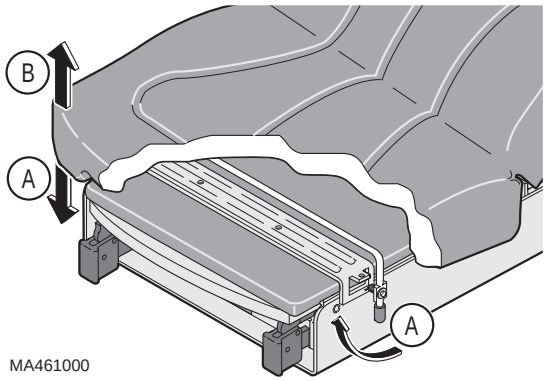

A. While rotating the pelvic lift bar, lower the seat.
B. Slightly raising the seat allows the spring loaded pelvic lift bar to snap to an upright position.

MIDMARK®
Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

003-0530-00 Rev. C (7/98)

© Midmark Corporation - 1998